





中国认可 国际互认 检测 TESTING CNAS L0599

Test Report SL52025269243701TX Date:June 22,2020 Page 1 of 4

HANGZHOU SHIJIE HEALTH TECHNOLOGY CO.,LTD NO 428 QIANZHANGZIRANG VILLAGE,HUANGJIAZHANG,SHUSHAN STREET,XIAOSHAN DISTRICT,HANGZHOU,ZHEJIANG,CHINA

The following sample(s) was/were submitted and identified on behalf of the client as:

Sample Description : (A)Disposable Medical Face Mask

Style No. : SJM206

Composition : (A)Non-woven fabric, Melt-blown fabric

Sample Color : (A)blue

Manufacturer : HANGZHOU SHIJIE HEALTH TECHNOLOGY CO.,LTD

Lot No./Batch No. : Not provided

Proposed Care Instruction: /

Test Performed : Selected test(s) as requested by applicant

Sample Receiving Date : Jun 01, 2020

Testing Period : Jun 01, 2020 - Jun 22, 2020

Test Result(s) : Unless otherwise stated the results shown in this test report refer only to the

sample(s) tested, for further details, please refer to the following page(s).

Signed for and on behalf of

SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd Testing Center

Sara Guo (Account Executive)

Janya - riela

Dongjing Liu / Hailian Xuan (Authorized Signatory)



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com/en/Terms-and-Conditions.aspx and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's ersponsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 83071443, or, email: CN.Doccheck@sgs.com

3[™]Building,No.889,Yishan Road,Xuhui District Shanghai,China 200233 中国・上海・徐汇区宜山路889号3号楼 邮編: 200233 t (86-21) 61402666 t (86-21) 61402666 f (86-21) 64958763 f (86-21) 64958763 www.sgsgroup.com.cn e sgs.china@sgs.com



Test Report

SL52025269243701TX

Date:June 22,2020

Page 2 of 4

Test Result

EN 14683:2019+AC:2019 Medical Face Masks-Requirements and Test Methods

Clause 5.2 Performance Requirement

Clause 5.2.2 Bacterial filtration efficiency (BFE)

(EN 14683:2019+AC:2019 Annex B)

Sample: A

Conditioning Parameters : Minimum of 4 hours at 21±5°C and 85±5% R.H.

Dimensions of test specimen : 170 mm x 160 mm

Test Area : ~60 cm²
Test Side : Inside
Flow Rate : 28.3 l/min
Positive Control Average : 2306.5 CFU
Negative Monitor Count : < 1 CFU

1# 2# 3# 4# 5# (BFE), % 99.9 99.9 99.9 99.9

Remark: Performance Requirement: Type I≥95%, Type II≥98%, Type IIR ≥98%

Clause 5.2.3 Breathability

(EN 14683 :2019+AC:2019 Annex C)

Sample: A

Test number and location : 5 random areas for each specimen (face mask) Conditioning Parameters : Minimum of 4 hours at 21±5°C and 85±5% R.H.

Test Area : 4.9 cm²
Flow Rate : 8 l/min

Remark: Performance Requirement: Type I<40 Pa/cm², Type II<40 Pa/cm², Type IIR<60 Pa/cm²



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com/en/Terms-and-Conditions.aspx and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's ersponsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 83071443, or, email: CN.Doccheck@sgs.com

3^{rg} Building,No.889,Yishan Road,Xuhui District Shanghai,China 200233 中国・上海・徐汇区宜山路889号3号楼 邮编: 200233 t (86-21) 61402666 f (86-21) 64958763 t (86-21) 61402666 f (86-21) 64958763 www.sgsgroup.com.cn e sgs.china@sgs.com



Test Report

SL52025269243701TX

Date:June 22,2020

Page 3 of 4

Clause 5.2.4 Splash Resistance

(ISO 22609 :2004, Pressure 16.0 kPa)

Penetration on inside surface										
1#	2#	3#	4#	5#	6#	7#	8#			
Pass	Pass	Pass	Pass	Pass	Pass	Pass	Pass			
9#	10#	11#	12#	13#	14#	15#	16#			
Pass	Pass	Pass	Pass	Pass	Pass	Pass	Pass			
17#	18#	19#	20#	21#	22#	23#	24#			
Pass	Pass	Pass	Pass	Pass	Pass	Pass	Pass			
25#	26#	27#	28#	29#	30#	31#	32#			
Pass	Pass	Pass	Pass	Pass	Pass	Pass	Pass			
Number of Pass:			32							
Overall result:			Acceptable							

Remark:

- 1) Performance Requirement Type I: N/A, Type II: N/A, Type IIR: ≥16.0kPa
- Distance of the medical face mask target area surface to the tip of cannula is 300±10mm.
- Condition and Test temperature (21±5)° C, relative humidity (85±10)%
- An acceptable quality limit of 4.0% is met for a single sampling plan when 29 or more of the 32 tested specimens show pass results

Clause 5.2.5 Microbial Cleanliness

(EN 14683:2019+AC:2019 Annex D and EN ISO 11737-1:2018)

	1#	2#	3#	4#	5#
CFU/g	14	24	41	16	33

Remark: Performance Requirement: Type I≤30 CFU/g, Type II≤30 CFU/g, Type IIR≤30 CFU/g



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com/en/Terms-and-Conditions/Terms

3rdBuilding,No.889,Yishan Road,Xuhui District Shanghai,China 200233 中国・上海・徐汇区宜山路889号3号楼 邮编: 200233

t (86-21) 61402666

t (86-21) 61402666 f (86-21) 64958763 f (86-21) 64958763 e sgs.china@sgs.com




Test Report

SL52025269243701TX

Date:June 22,2020

Page 4 of 4

Sample Photo

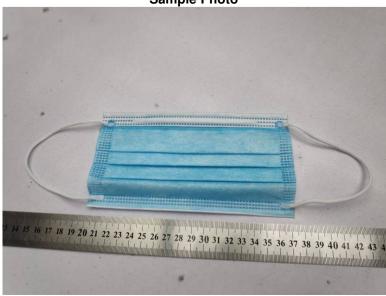

The statement of conformity in this test report is only based on measured values by the laboratory and does not take their uncertainties into consideration.

End of Report



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com/en/Terms-and-Conditions/Terms

3stBuilding,No.889,Yishan Road,Xuhui District Shanghai,China 200233 中国 • 上海 • 徐汇区宜山路889号3号楼 邮编: 200233 t (86-21) 61402666 t (86-21) 61402666

f (86–21) 64958763 f (86–21) 64958763 www.sgsgroup.com.cn e sgs.china@sgs.com